


FTT Single Burning Item (SBI)

(EN 13823)

firetesting
technology

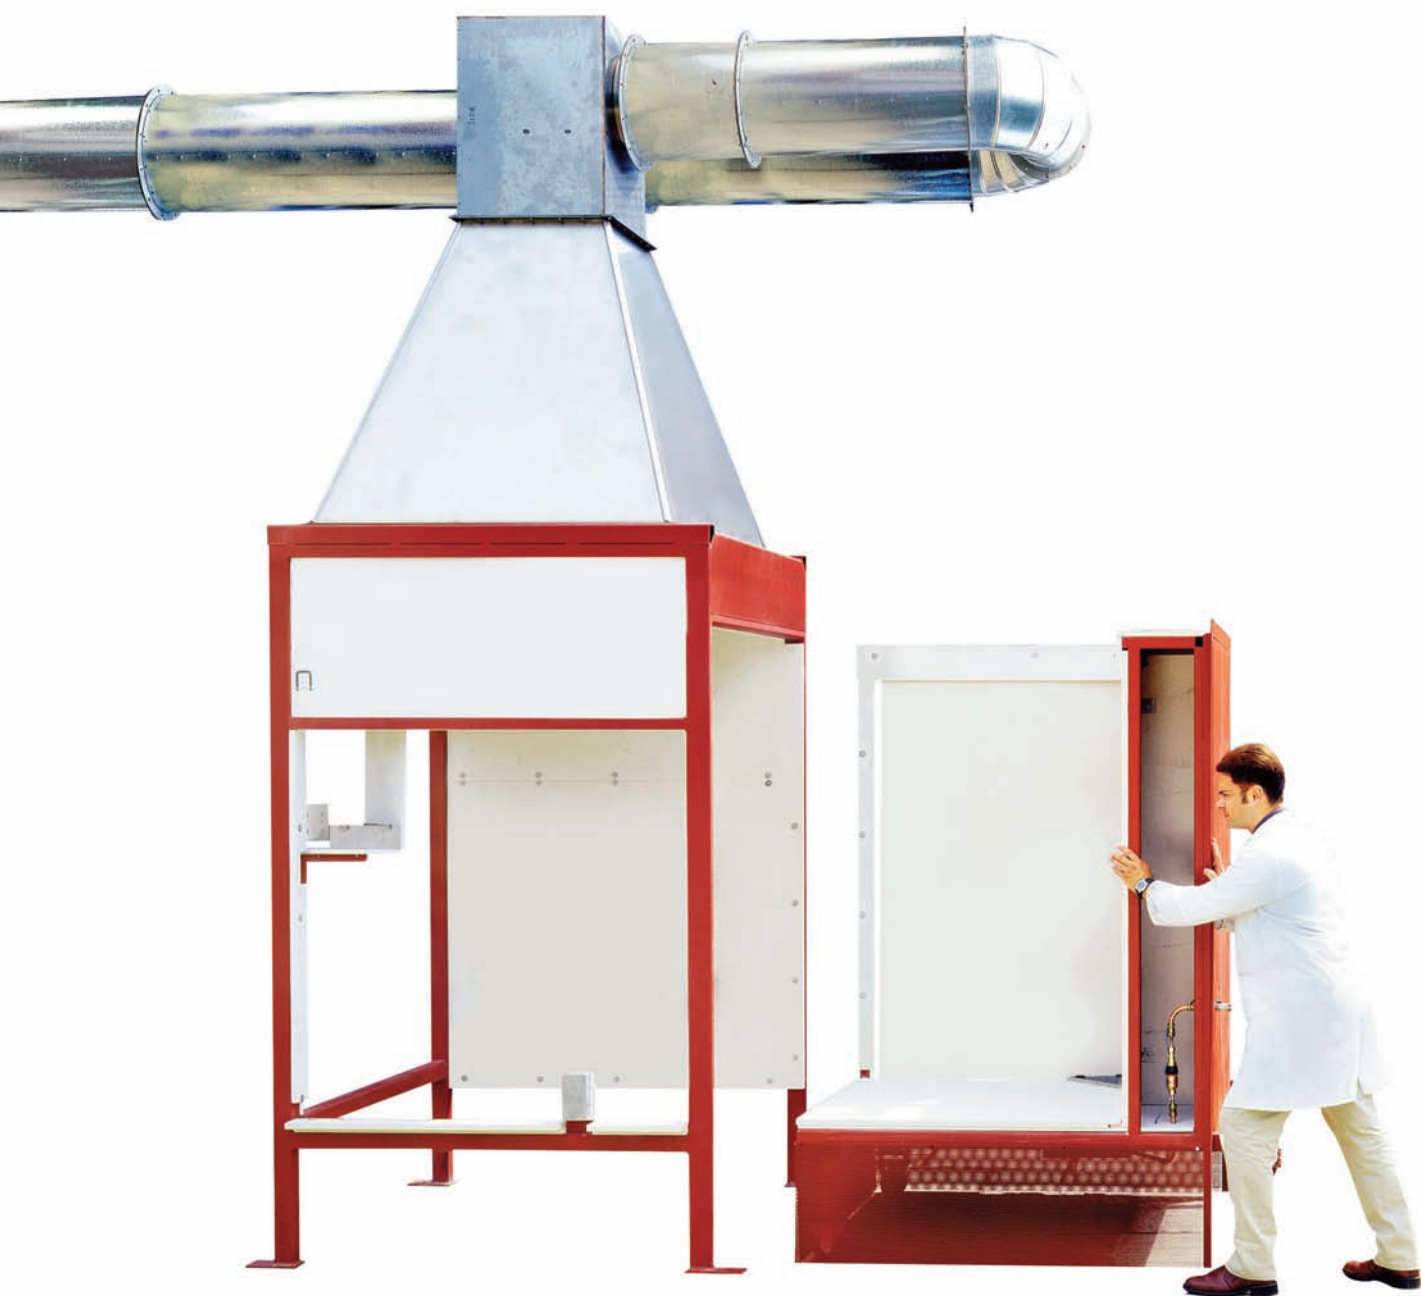

EN 13823:

Reaction to fire tests for building products excluding floorings exposed to thermal attack by a single burning item, the SBI.

The importance of the SBI

The European Construction Products Regulation requires that all European Member states use this test method to evaluate reaction to fire performance for all construction products excluding flooring. These test methods will eventually take precedence over national regulatory methods to classify most building products and will be required by all suppliers of building materials into the EU and neighbouring states adopting these regulations.

The SBI Test

The Single Burning Item (SBI), is a method of test for determining the reaction to fire behaviour of building products (excluding floorings) when exposed to the thermal attack from a single burning item (modelled by a

propane fuelled sand-box burner). The specimen is mounted on a trolley that is positioned in a frame beneath an exhaust system. The reaction of the specimen to the burner is monitored instrumentally and visually. Heat and smoke release rates are calculated and physical characteristics are assessed by observation. The parameters that are quantified in this test and used within the classification criteria are Total Heat Release (THR), Fire Growth Rate Index (FIGRA) and Smoke Growth Rate index (SMOGRA).

How the SBI is used to classify products


The European Commission recently defined the classification criteria for building products. These performance classes range from A to F. Although other test methods are required for assessment, SBI testing is needed to classify all non flooring products qualifying for classes A2, B, C and D, which are the major classes inhabited by most products other than those that are principally inorganic and classified as non-combustible (A1).

The FTT SBI

FTT supplies and installs the apparatus and train clients in its use. **FTT** can also supply any of the components to clients wishing to part design and build their own equipment.

The main components of the **FTT** SBI are:

- Frame, trolley, hood and ducting.
- Gas analysis instrumentation for heat release measurement.
- Smoke measurement system.

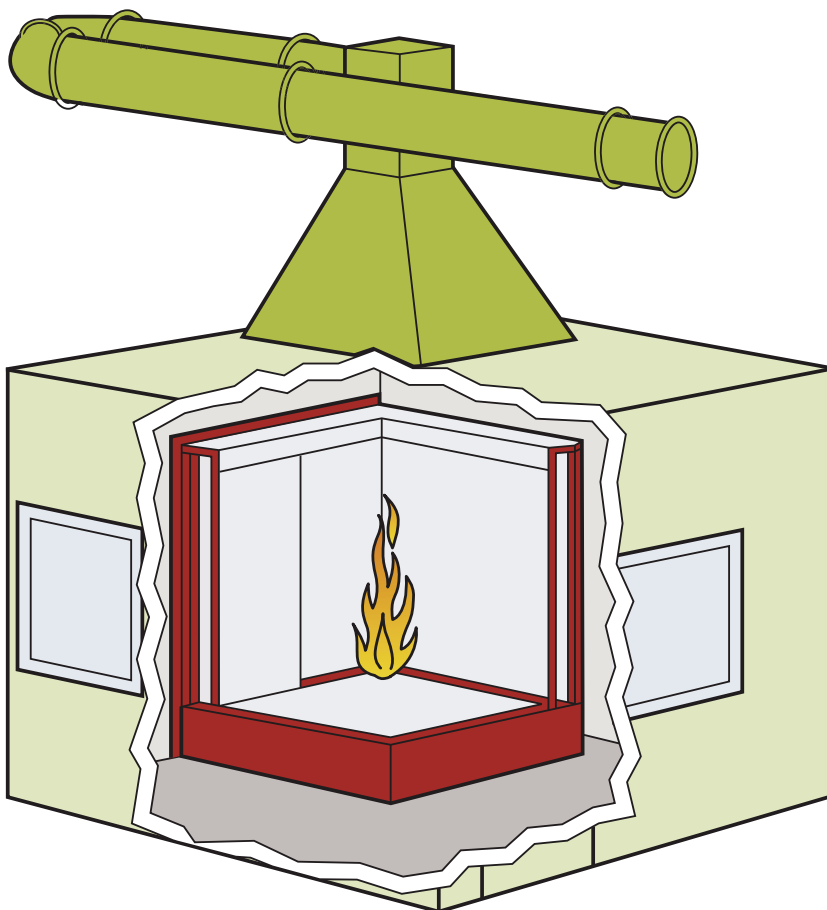

CLASS	CLASSIFICATION CRITERIA	ADDITIONAL CLASSIFICATION	OTHER TEST METHOD(S)
A2	FIGRA \leq 120W/s; and LFS < edge of specimen; and THR _{600s} \leq 7.5 MJ	Smoke production; and Flaming droplets/particles	EN ISO 1716
B	FIGRA \leq 120W/s; and LFS < edge of specimen; and THR _{600s} \leq 7.5 MJ	Smoke production; and Flaming droplets/particles	EN ISO 11925-2
C	FIGRA \leq 250W/s; and LFS < edge of specimen; and THR _{600s} \leq 15 MJ	Smoke production; and Flaming droplets/particles	EN ISO 11925-2
D	FIGRA < 750W/s	Smoke production; and Flaming droplets/particles	EN ISO 11925-2

- Burner, gas train and controls.
- Data acquisition and analysis software.

Test apparatus includes:

- Trolley, which holds the specimen and which docks into the frame.
- Primary and secondary burners.
- Frame, which is built into the test room.
- Collector with baffles, fitted to the hood.
- Ducting with guide vanes.
- Duct section containing gas sampling probe, bi-directional probe and thermocouples for mass flow measurement and smoke measuring ports.



The FTT SBI frame trolley

Gas Analysis Instrumentation

Housed in a 19" rack containing:

- **FTT** Calorimeter Analyser featuring Paramagnetic oxygen sensor with atmospheric pressure compensation and Infrared carbon dioxide sensor (0-10%). Carbon monoxide (0-1%) is optional.
- Developed and optimised specifically for the **FTT** calorimeters this analyser features flow control and bypass for fast response, low drift and noise and is compatible with small, medium and large calorimeters.
- Soot filter, refrigerant cold trap, drying column(s), pump and waste regulators for conditioning the sampled gases prior to analysis.
- Controls for the smoke measurement system (if purchased).



19" Gas Analysis Rack

Clients owning an **FTT** Dual Cone Calorimeter can use the instrument rack from the cone for this function. Similarly clients purchasing this equipment will own a substantial section of a **FTT** Dual Cone Calorimeter and later be able to purchase a Cone Calorimeter with significant savings.



Smoke Measurement System

Includes:

- White light source and lens built in accordance with DIN 50055.
- Silicon photodiode detector and voltage output of transmission
- SBI support cradle
- Full set of calibration filters.
- Analysis is via software.


Burner, Gas Train and Controls

Includes:

- Two non-aerated sandbox burners and an ignition system.
- UV burner flame detector units for safe gas supply monitoring.
- ‘Gas Control Box’, housed next to the test room observation window so the operator can simultaneously see the test specimen and digital propane mass flow rate (mg/s). This unit includes three flow level controllers, warning lights and override facilities.
- ‘Gas Diverter’ consisting of a mass flow controller to control the propane gas flow. Solenoid valves and flash back arrestors in both gas supply lines for automated safe operation of the gas flow to the burners. These are housed close to the test frame to improve the response time of the burners by reducing the pipe length between the solenoids and burners. The propane mass flow rate and the corresponding heat release (kW) are additionally displayed via software.



Gas Control Box

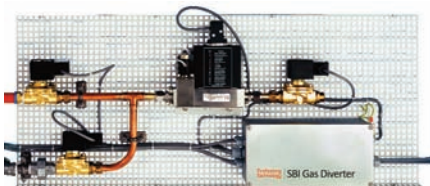

Gas Diverter



Data acquisition and analysis

Includes:

- A Windows based software package enabling simple data collection and manipulation to determine the various parameters needed for heat release determination. The software generates files that integrate with the current spreadsheets, (which are also supplied) for the calculation of the Fire Growth Rate Index (FIGRA) and Smoke Growth Rate Index (SMOGRA).
- Data logger, which features a 3-slot cardcage with 6 1/2 digit (22 bit) internal DMM enabling up to 120 single-ended or 48 double-ended measurements, collects signals from the instrumentation. Scan rates up to 250 channels/s are available with a 115 kbaud RS232 interface as standard. Also supplied with GPIB interface.

Software

Instrument supplied with software at no extra charge. Software updates provided free of charge.

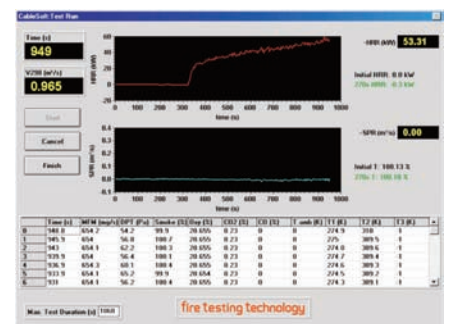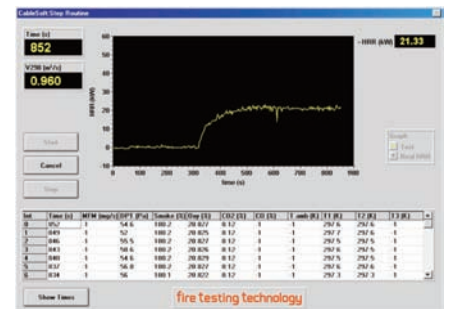

Services required for complete installation of an SBI

FTT supplies all instrumentation and ducting for the SBI and can help with laboratory design, supplying of additional items or supervision of local building works or installation of essential services. The test may produce large quantities of combustion products so smoke handling facilities and suitable extinguishing agents are recommended.

You will also need:

- Minimum height of 4.5m to house full apparatus
- Minimum floor space required (3m × 3m)
- Extraction (0.5m³/s to 0.65m³/s)
- Air supply
- Oxygen-free nitrogen
- Drying agents
- Calibration gas of CO₂/nitrogen (and CO if this option is purchased)
- Commercial propane supply
- Electrical power providing 230VAC 50/60 Hz 16A at the instrument rack must be available.

Other Euroclass test methods

To classify the reaction to fire of the full range of wall lining and flooring construction products, the SBI and up to 4 other European Standard test methods may be required. **FTT** supplies instrumentation complying with all these European Standard test methods.

The test methods are:

- Single-Flame Source Test
EN ISO 11925-2. Reaction to fire tests for building products – Ignitability of building products subjected to direct impingement of flame.
- Oxygen Bomb Calorimeter
EN ISO 1716. Reaction to fire tests for building products – Determination of the heat of combustion.
- Non Combustibility Apparatus
EN ISO 1182. Reaction to fire tests for building products – Non combustibility test.
- Flooring Radiant Panel
EN ISO 9239-1. Reaction to fire tests for building products – Horizontal surface spread of flame for floor coverings.

TECHNICAL SPECIFICATIONS	
Measuring Principle	Paramagnetic oxygen analysis. Infrared carbon dioxide analysis.
System Dimensions (mm)	
Trolley	1500 (W) × 1620 mm (D) × 2200mm (H)
Frame	1500(W) × 1700 mm (D) × 2500mm (H)
Ducting	315 internal diameter (to length and specification as per Standard)
Gas flow rate (for burner)	647 mg/s and 2000 mg/s
Smoke detector	Silicon photodiode detector
Software	Windows based data acquisition and analysis

Due to the continuous development policy of **FTT** technical changes could be made without prior notice.

Unrivalled Experience in Design and Manufacturing

FTT's site in East Grinstead, is home to the largest group of fire scientists and instrumentation design engineers working on fire testing instrumentation, and is at the heart of our design and manufacturing. For more than 30 years FTT has provided the highest quality instruments and service for fire testing and research professionals worldwide, directly and through its extensive global sales and support network.



Quality

- World-class manufacturing in accordance with multiple international and national standards, including: EN, ISO & ASTM
- ISO 9001, ISO 14001 certified

Integrity

- A dedicated team passionate about fire testing instrumentation and continuous product improvement
- Delivering reliable, robust and easy-to-use instruments for the past 30 years

Excellence

- A world-class team made up of qualified fire scientists, mechanical, electrical and electronic fire instrument design engineers and production, installation and maintenance engineers

Global

- World-wide distribution network for global sales, installations, training, maintenance and technical support
- Leading global supplier of the Cone Calorimeter, Large Scale Calorimeter, NBS Smoke Chamber and Oxygen Index